



Indian Standard


(Reaffirmed 1998)

(Reaffirmed 2013)

SPECIFICATION FOR OCCLUSAL PLANE GUIDE, DENTAL

1. Scope — Dimensions and other requirements for occlusal plane guide used in dentistry.

2. Shape and Dimensions — As shown in Fig. 1.

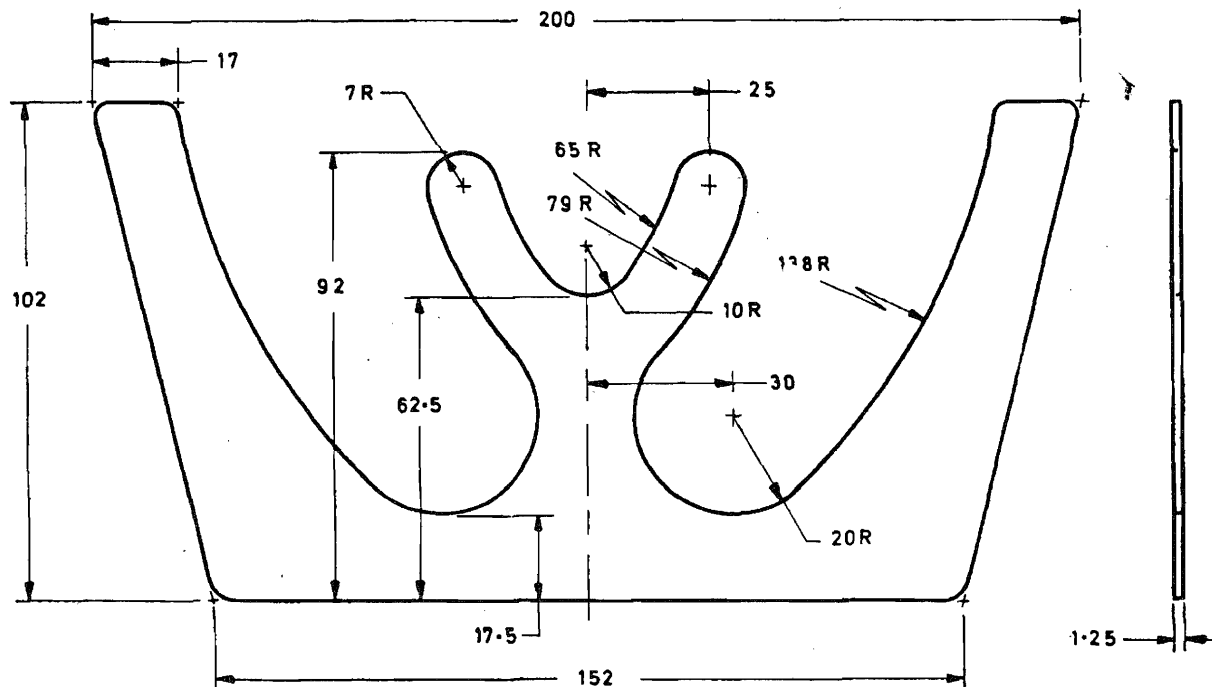

All dimensions in millimetres.

FIG. 1 OCCLUSAL PLANE GUIDE, DENTAL

3. Material — Wrought aluminium alloy sheet conforming to Designation NS5 of IS : 737-1965 'Specification for wrought aluminium and aluminium alloys, sheet and strip (for general engineering purposes) (revised) '.

4. Workmanship and Finish

4.1 The instrument shall be absolutely flat and shall remain so during the normal use. The edges shall be suitably radiused.

4.2 The instrument shall be free from surface defects and shall have mat finish.

5. Marking — The plane guide shall be marked with the manufacturer's name, initials or recognized trade-mark; and the country of manufacture.

5.1 ISI Certification Marking — Details available from the Indian Standards Institution, New Delhi 1.

6. Packing — The plane guide shall be wrapped in moisture-proof paper or packed in polyethylene bag.

Adopted 2 September 1970

© February 1971

ISI Price Rs. 1.00

INDIAN STANDARDS INSTITUTION
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 1

MAX. RETAIL PRICE
INCL. OF ALL TAXES
890